
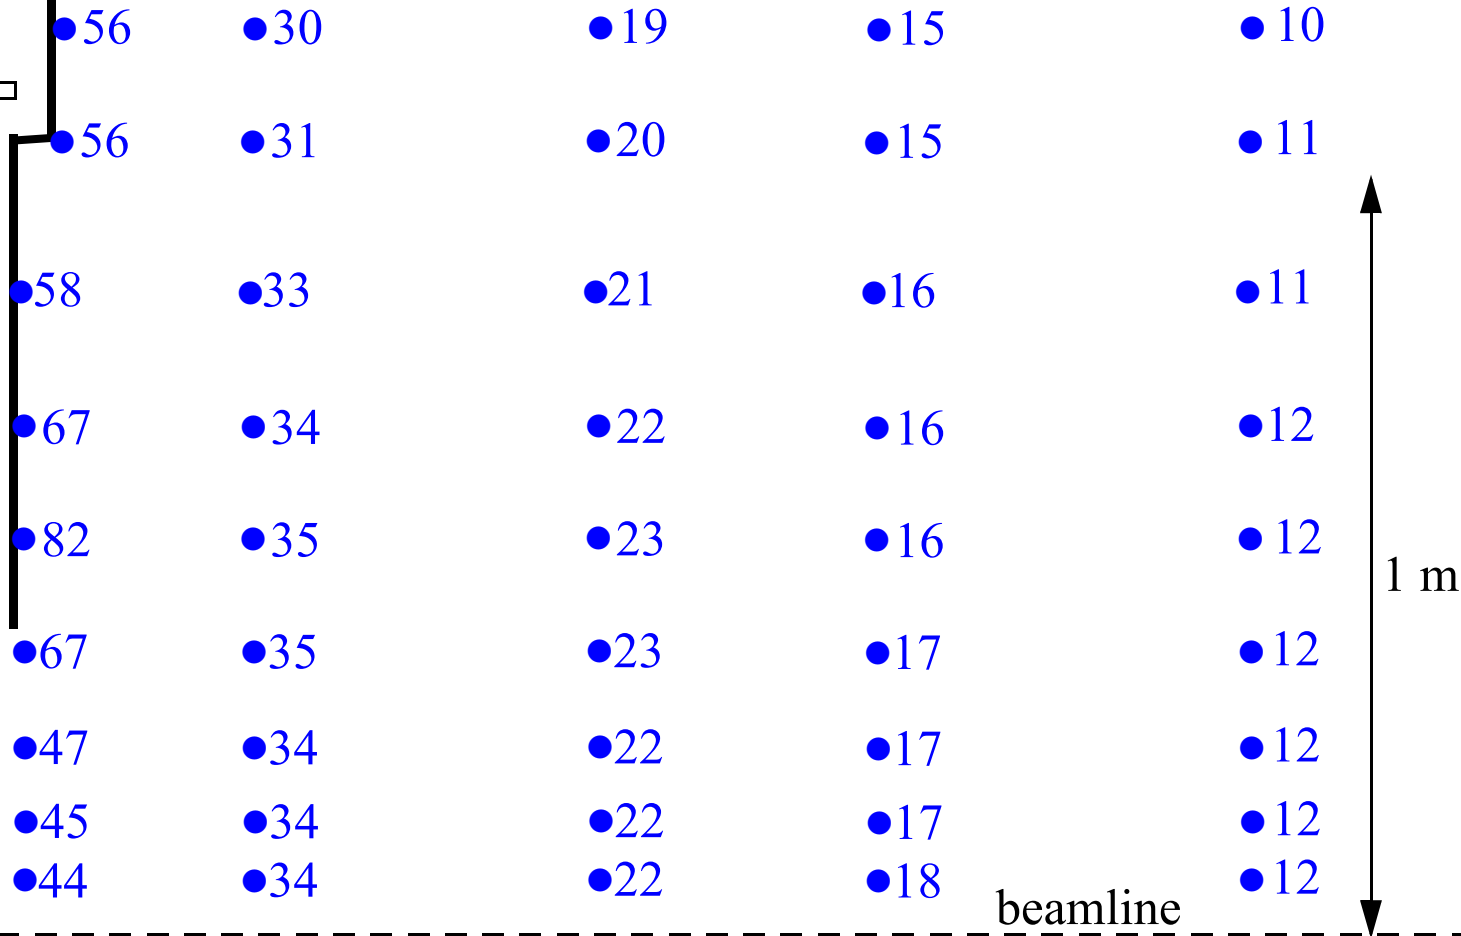


LAr Calorimeter

Dose rates in $\mu\text{Sv/h}$ from the beampipe, the inner detector and the LAr calorimeter after 10 years of running and 5 days of cooling.

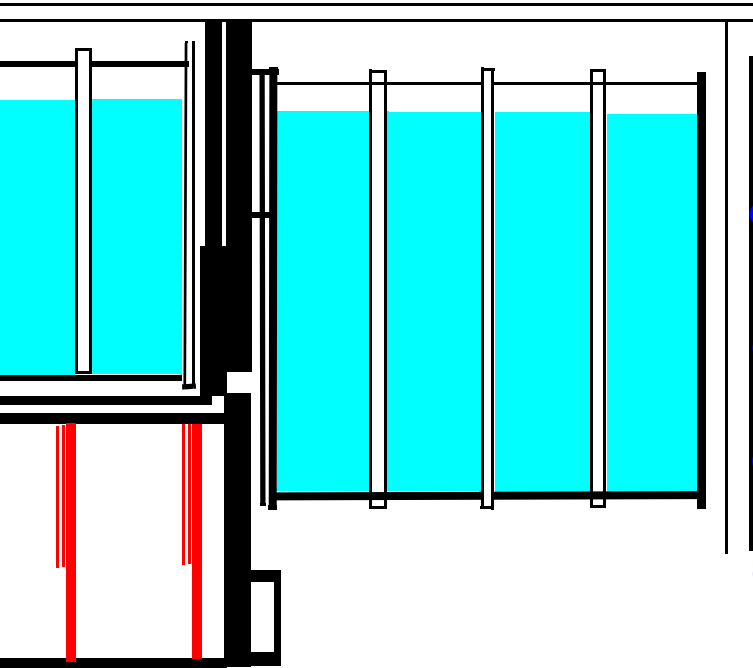

Pixel detector removed

beamline

1 m

1 m